

Instruction Manual

Stratos PROFIBUS 2221 X Oxy

Knick >

Warranty

Defects occurring within 3 years from delivery date shall be remedied free of charge at our plant (carriage and insurance paid by sender).

Accessories: 1 year

Software release: 2.x

Date of issue: 20070810



Contents

1	Information on this instruction manual	3	7	Commissioning	20
	Markings	3		Checklist	20
2	Safety information	4	8	Operation	21
	Be sure to read and observe the following instructions!	4		Operation possibilities	21
3	PROFIBUS technology	5		Operation using keypad on the device	22
	General	5		Mode code	24
	Variants and basic characteristics	5		Safety functions	24
	Definitions for PROFIBUS-PA	6		Mode indicators	25
	PROFIBUS-PA with Stratos	6		Configuration	E-26
4	Description	7		Calibration	29
	Proper use	7		Operating tool	E-35
	Technical features	7		Measurement	35
	Communication model	8	9	Diagnostics	36
	Profile for process control devices (extract)	9		Sensocheck, Sensoface	36
5	Assembly	11		PROFIBUS-PA limit monitoring	37
	Package contents and unpacking	11		Error messages	E-38
	Mounting plan	12		Display messages and PROFIBUS communication	40
6	Installation and connection	15		Diagnostics functions	E-43
	Information on installation	15	10	Maintenance and cleaning	45
	Terminal assignments	17		Maintenance	45
	Overview of the Stratos	17		Cleaning	45
	Dissolved oxygen measurement	18	11	Appendix	46
				Product line	46

Specifications	46
ATEX EC-Type-Examination Certificate	51
Declaration of Conformity	54
FM Control Drawing	55
12 Index	57

1 Information on this instruction manual

1.1 Markings



The warning symbol means that the instructions given must always be followed for your own safety.

Failure to follow these instructions may result in injuries



Notes provide important information that should be strictly followed when using the device.



When a key is shown, its function is explained.



When a display is shown, the corresponding information or operating instructions are provided.

Operating instructions

- Each operating instruction is preceded by a dot.

Enumerations

- Each enumeration is preceded by a dash.

Model designation

For practical purposes, the Stratos PROFIBUS 2221 X Oxy is simply referred to as Stratos in this instruction manual.

Trademarks

The following names are registered trademarks. For practical reasons they are shown without trademark symbol in this manual.

- Registered trademarks
 - Stratos®
 - Sensocheck®
 - Sensoface®
 - Calimatic®
 - GainCheck®
 - InPro®

InPro® is a registered trademark of Mettler Toledo.

2 Safety information

2.1 Be sure to read and observe the following instructions!

The device has been designed in accordance with the state of the art and complying with the applicable safety regulations.

When operating the device, certain conditions may nevertheless lead to danger for the operator or damage to the device.



Whenever it is likely that protection has been impaired, the device shall be made inoperative and secured against unintended operation.

The protection is likely to be impaired if, for example:

- the device shows visible damage
- the device fails to perform the intended measurements
- after prolonged storage at temperatures above 70 °C
- after severe transport stress

Before recommissioning the device, a professional routine test in accordance with EN 61010-1 must be performed. This test should be carried out by the manufacturer.



Stratos PROFIBUS 2221 X Oxy is approved for installation in ATEX, FM Zone 1 with measurement in Zone 0, and FM Class I Div 1.

Before commissioning it must be proved that the intrinsic safety is maintained when connecting the device to other equipment, such as segment coupler and cable.



For hazardous-area applications, the Stratos PROFIBUS 2221 X Oxy may only be connected to explosion-proof segment couplers, power supplies

The Stratos PROFIBUS 2221 X Oxy may be operated in accordance with the FISCO model.



The stipulations of EN 60079-10: 1996 and the following must be observed for the installation.



In hazardous locations the Stratos may only be cleaned with a damp cloth to prevent electrostatic discharge.

3 PROFIBUS technology

3.1 General

PROFIBUS is a digital communication system that connects different field devices over a common cable and integrates them into a control system. In the long term, PROFIBUS will replace the 4-20 mA technology, which only supplies pure measured values.

Advantages of the PROFIBUS technology are:

- easy and cost-saving cabling
- convenient operation over a central control station
- transmission, evaluation and control of high amounts of data from field device to control station.

- devices installed in hazardous locations are configured and maintained from the control station

PROFIBUS is the leading open fieldbus system in Europe. Its application range covers manufacturing, process and building automation. As open fieldbus standard to EN 50170, PROFIBUS ensures communication of different devices over one bus.

The PROFIBUS User Organization (PNO) provides for further development and maintenance of the PROFIBUS technology. It combines the interests of users and manufacturers.

English

3.2 Variants and basic characteristics

PROFIBUS determines the technical and functional characteristics of a serial bus system.

There are three PROFIBUS variants:

- PROFIBUS-FMS (FMS protocol)
 - is particularly suited for exchanging large amounts of data between control devices. It operates according to the RS 485 standard with transmission rates up to 12 Mbits/sec.
 - PROFIBUS-DP (decentralized peripherals)
 - is tailored for communication of automation systems and distributed peripherals. It operates according to the RS 485 standard with transmission rates up to 12 Mbits/sec.
 - PROFIBUS-PA (process automation)
 - is dedicated to the process industry. It permits connection of sensors and actuators to a common bus even in hazardous locations. PROFIBUS-PA has a transmission rate of 31.25 kbits/sec.
- Masters
 - control the data traffic on the bus. They send messages without external request.
 - Slaves
 - are peripheral devices such as valves, drives, transmitters and analyzers. They can react acyclically to servicing, configuration and diagnostic tasks of the master. The central controller cyclically reads the measurement data with status.

PROFIBUS distinguishes between two types of devices:

3.3 Definitions for PROFIBUS-PA

The bus protocol defines type and speed of the data exchange between master and slave devices and determines the transmission protocol of the respective PROFIBUS system.

PROFIBUS-PA permits cyclic and acyclic services.

- Cyclic services are used for transmission of measurement data and actuating commands with status information.

- Acyclic services are used for device configuration, maintenance and diagnostics during operation.

The device profile defines the device class and typical functionalities with parameters, ranges and limit values.

The FISCO model developed by the German PTB for hazardous locations permits connection of several devices to one common bus and defines permissible limits for device and cable parameters.

3.4 PROFIBUS-PA with Stratos

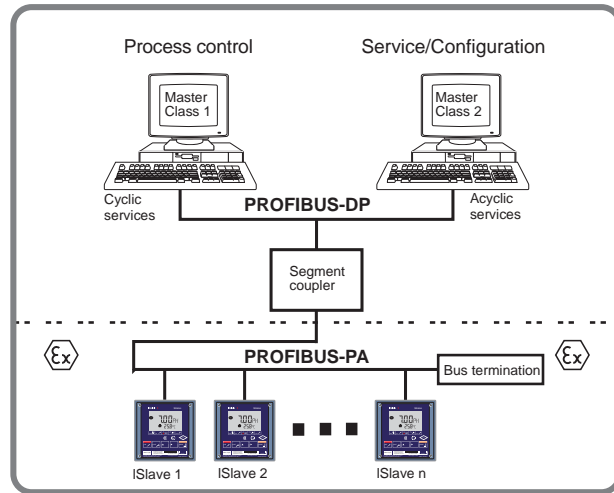


Fig. 3.1 Typical configuration of a PROFIBUS system with Stratos

4 Description

4.1 Proper use

Stratos is a PROFIBUS-PA analyzer. The Stratos is used for dissolved oxygen and temperature measurement in biotechnology, pharmaceutical industry, as well as in the field of environment, food processing and sewage treatment.

The rugged molded enclosure can be wall mounted or fixed into a control panel. It can also be mounted at a post or pipe.

The protective hood provides additional protection against direct weather exposure and mechanical damage.

The unit can be easily replaced since the terminals are of a plug-in design.

The Stratos has been designed for application with amperometric sensors.

English

4.2 Technical features

Communication between measuring point and control room is via PROFIBUS-PA. The data exchange (cyclic and acyclic) is performed

in accordance with the PROFIBUS-DP/V1 protocol.

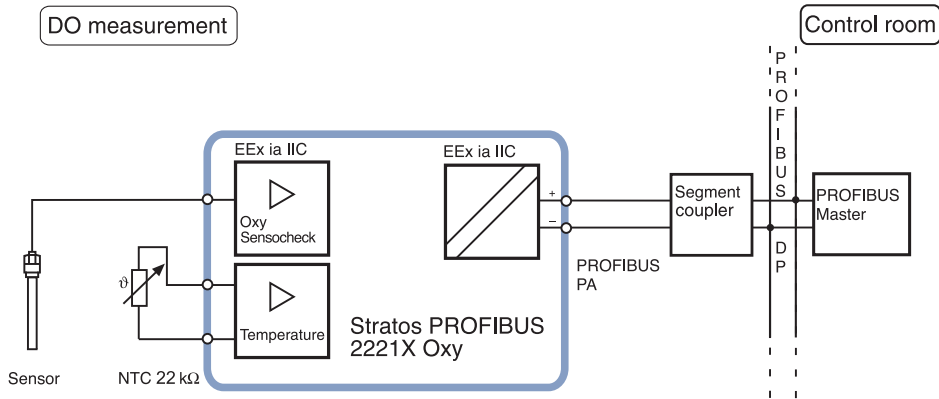


Fig. 4.1 System functions (hardware)

4.3 Communication model

The device performance is described by function blocks according to the PNO profile for Process Control Devices. The respective blocks contain different parameters and functions.

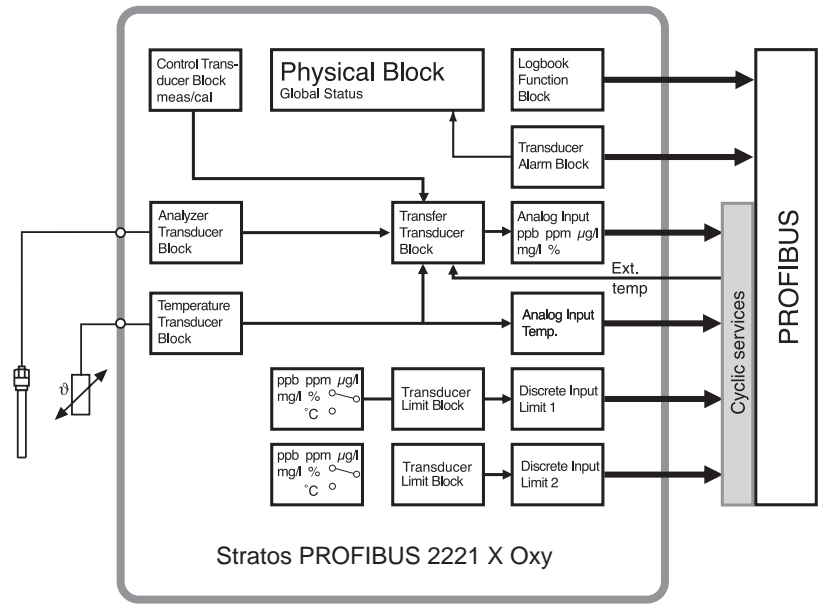


Fig. 4.2 Communication model Stratos PROFIBUS 2221 X Oxy according to the Profile for Process Control Devices (PNO)

4.4 Profile for process control devices (extract)

Type of block	Block contents (general)	Block contents (detailed)
Physical Block (PB)	Device description	Measurement procedure, device configuration Serial number, manufacturer name Operating state (run, maintenance, ...) Global status, diagnostics information
Transducer Block (TB)	Measurement procedure with interpretation	Process variable (plain text and unit) Number of measurement ranges (MR), start and end value of MR, active MR Sampling rate of measured values Uncorrected measured value with status
Control Transducer Block	Control of device functions	Status of function execution of respective Transducer Blocks Calibration data
Transfer Transducer Block	Pre-processing of a measured value	Measured value pre-processing Temperature compensation Selection of processing function
Transducer Limit Block	Limit monitoring	Block (TB) for limit setting Threshold, effective direction, hysteresis On-delay, off-delay Reset behavior, reset confirmation Limit status (active, not active)

English

Type of block	Block contents (general)	Block contents (detailed)
Analog Input (AI) Function Block	Measured value	Currently measured value with status and scale Rise time, hysteresis of AI limits Upper/lower alarm limit Upper/lower warning limit Switchover manual/automatic operation, measured value simulation Fail-safe behavior
Discrete Input (DI) Function Block	Digital input	Switchover manual/automatic operation Limit value message/status Signal inversion Fail-safe behavior
Transducer Alarm Block	Signaling of states and events	Required maintenance, function check, errors, limit values incl. summing
Logbook Function Block	Registration of states and events	Power on, power off, reset State of execution Navigation through entries

Tab. 4.1: Profile for Process Control Devices (function contents)

5 Assembly

5.1 Package contents and unpacking

Unpack the device carefully. Check the shipment for transport damage and completeness.

The package should contain:

- Front unit of Stratos
- Lower case

- This instruction manual
- Short instruction sheet
- Floppy disk with GSD file KNIC7533.GSD
- Bag containing small parts:

English


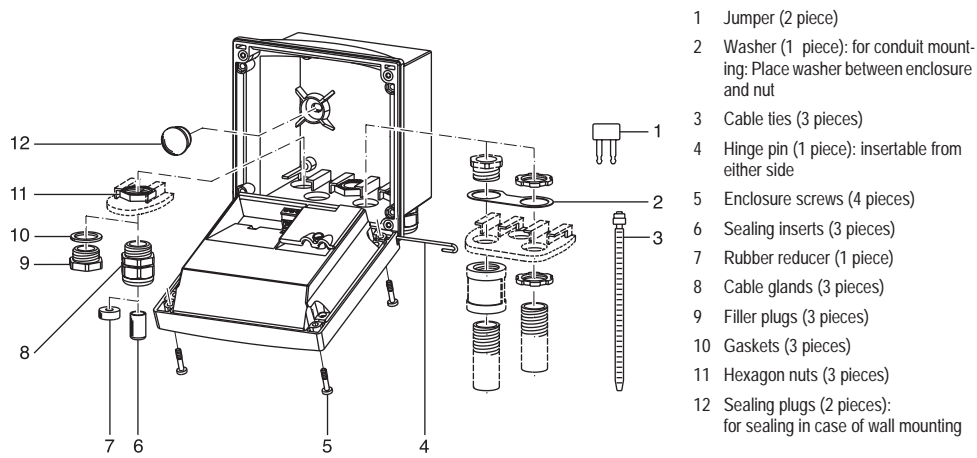



Fig. 5.1 Assembling the enclosure

5.2 Mounting plan

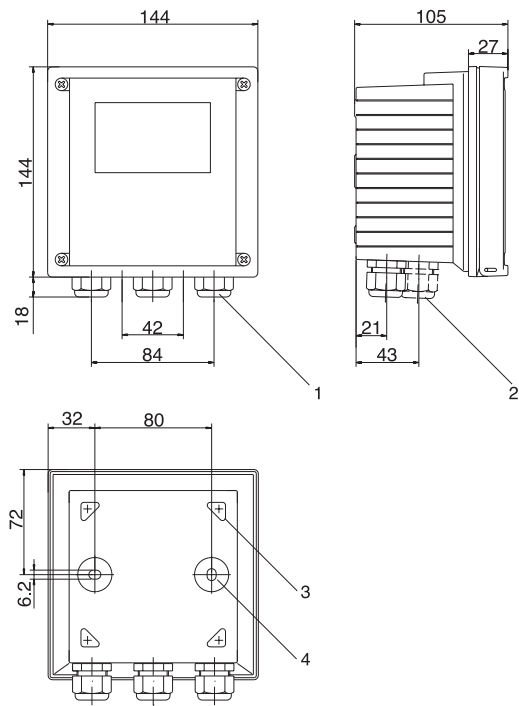


- 1 Cable gland
(3 pieces)
- 2 Breakthroughs for cable gland or
conduit 1/2", $\varnothing = 21.5$ mm
(2 breakthroughs)
Cable glands and conduits not
included!
- 3 Breakthroughs for pipe mounting
(4 breakthroughs)
- 4 Breakthroughs for wall mounting
(2 breakthroughs)

Fig. 5.2 Mounting plan

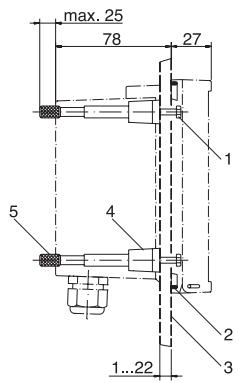

- 1 Screws (4 pieces)
- 2 Gasket (1 piece)
- 3 Panel
- 4 Span pieces (4 pieces)
- 5 Threaded sleeves (4 pieces)

Fig. 5.3 ZU 0275 panel-mount kit, panel cutout 138 x 138 mm (DIN 43700)

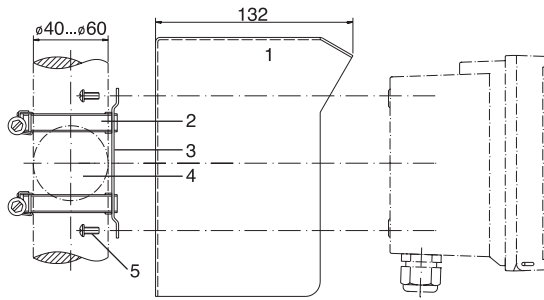

- 1 ZU 0276 protective hood (if required)
- 2 Hose clamps with worm gear drive to DIN 3017 (2 pieces)
- 3 Pipe-mount plate (1 piece)
- 4 For vertical or horizontal posts or pipes
- 5 Self-tapping screws (4 pieces)

Fig. 5.4 ZU 0274 pipe-mount kit

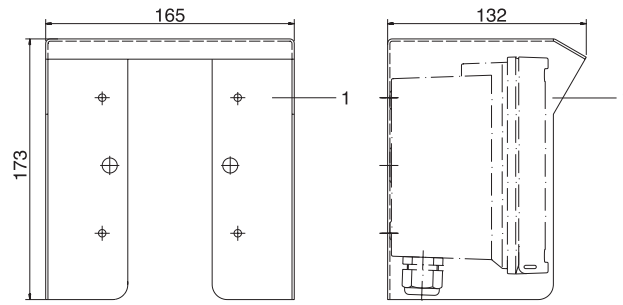


Fig. 5.5 ZU 0276 protective hood for wall and pipe mounting

6 Installation and connection

6.1 Information on installation



Installation may only be carried out by trained experts in accordance with this instruction manual and as per applicable local and national codes.



Be sure to observe the technical specifications and input ratings during installation.



According to the PTB FISCO model, the limits of the permissible parameter range must be observed for connection in a hazardous location.

See PROFIBUS Technical Guidelines PNO Order No.: 2.091




Be sure not to notch the conductor when stripping the insulation.

For easier installation, the terminal strips are of a plug-in design. The terminals are suitable for single wires and flexible leads up to 2.5 mm² (AWG 14).

A special twisted and shielded two-wire cable (e.g. Siemens) is used as bus cable.

Division 2 wiring


The connections to the Transmitter must be installed in accordance with the National Electric Code (ANSI-NFPA 70) Division 2 hazardous (classified) location non-incendive wiring techniques.

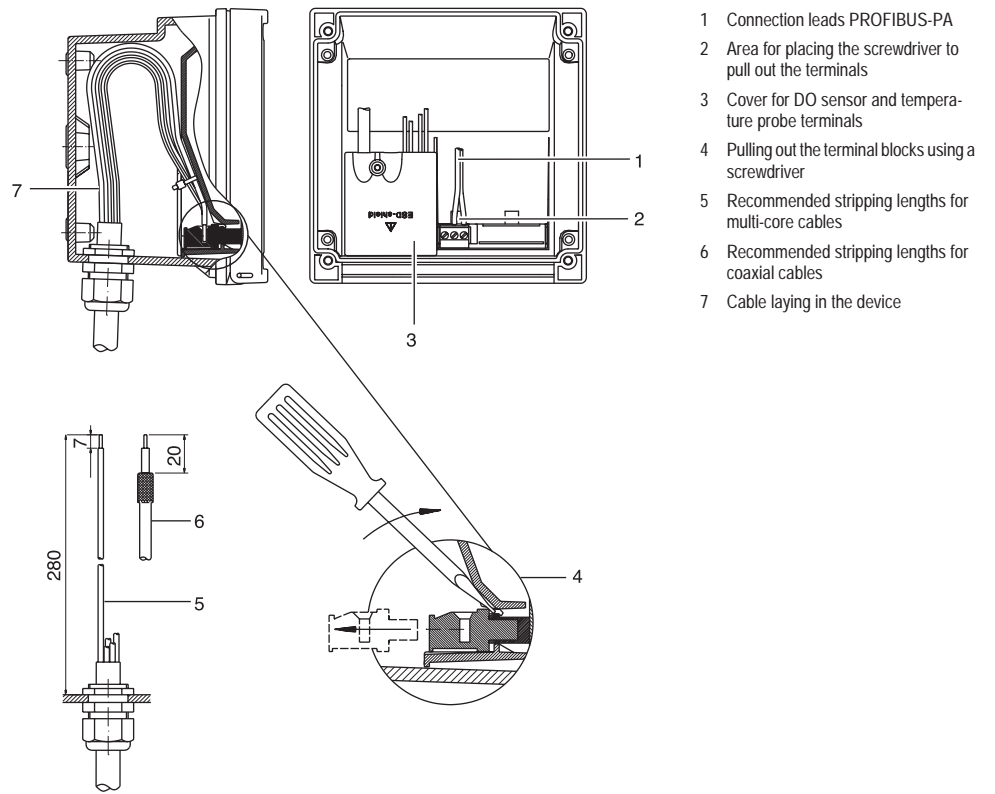

- 1 Connection leads PROFIBUS-PA
- 2 Area for placing the screwdriver to pull out the terminals
- 3 Cover for DO sensor and temperature probe terminals
- 4 Pulling out the terminal blocks using a screwdriver
- 5 Recommended stripping lengths for multi-core cables
- 6 Recommended stripping lengths for coaxial cables
- 7 Cable laying in the device

Fig. 6.1 Information on installation


6.2 Terminal assignments

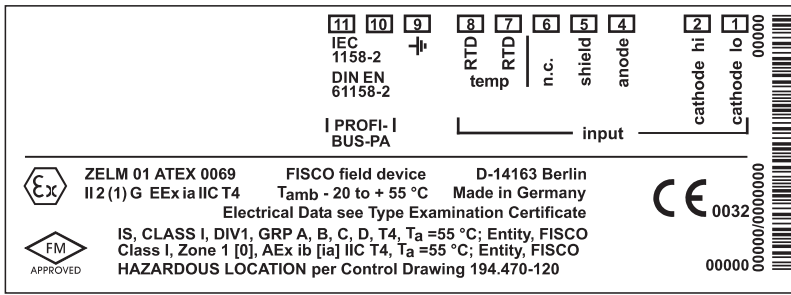

English

Fig. 6.2 Terminal assignments of Stratos

6.3 Overview of the Stratos

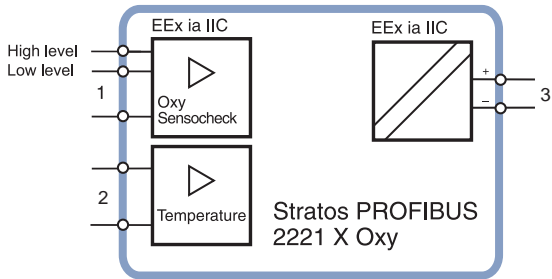

- 1 Inputs for 2 different DO sensors
- 2 Input for temperature probe
- 3 PROFIBUS-PA, protected against polarity reversal

Fig. 6.3 Inputs and outputs

A DO sensor
 B Temperature probe


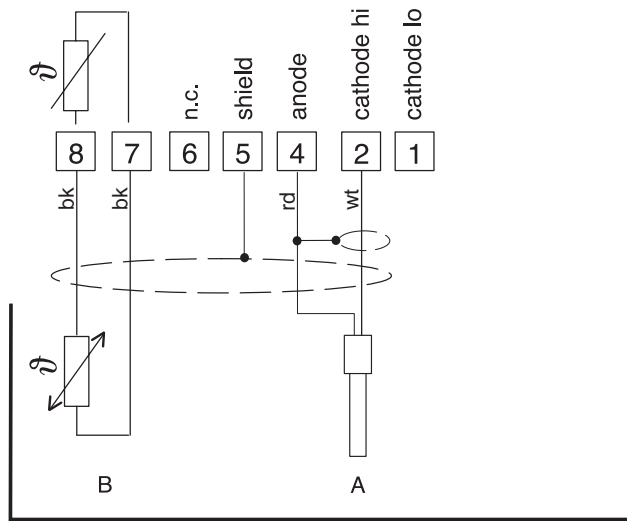


Fig. 6.4 Typical wiring of SE 704/705 or InPro 6000 sensors

- A DO sensor
- B Temperature probe

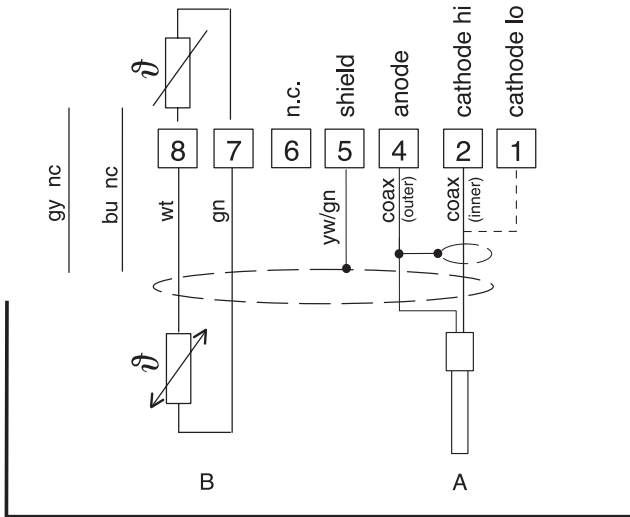

English

Fig. 6.5 Typical wiring of sensors with VP cable

7 Commissioning

7.1 Checklist



Commissioning may only be carried out by trained experts.



Before commissioning the Stratos PROFIBUS 2221 X Oxy, the following requirements must be met:

- The device must not show any damage.
- When recommissioning the device after a repair, a professional routine test in accordance with EN 61010-1 must be performed.
- It must be proved that the intrinsic safety is maintained when connecting the device to other equipment.
- It must be ensured that the device is configured in accordance with the connected peripherals.
- All connected voltage and current sources must correspond to the technical data of the device.
- The device must only be connected to explosion-proof segment couplers, power supplies, ...

8 Operation

8.1 Operation possibilities

English

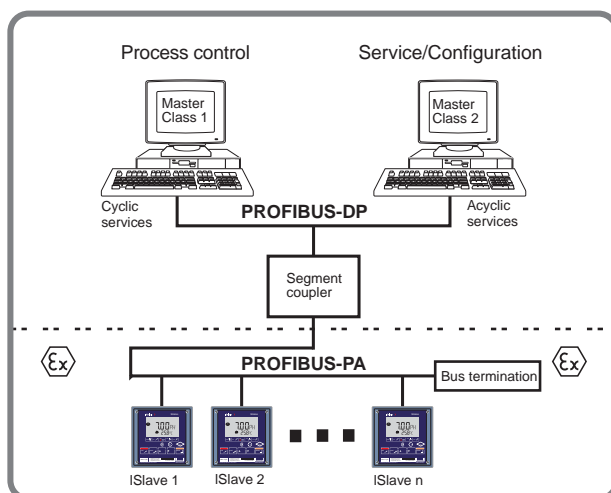


Fig. 8.1 System configuration

The device can be operated as follows:

- using the keypad on the device
- using an operating tool in the service station


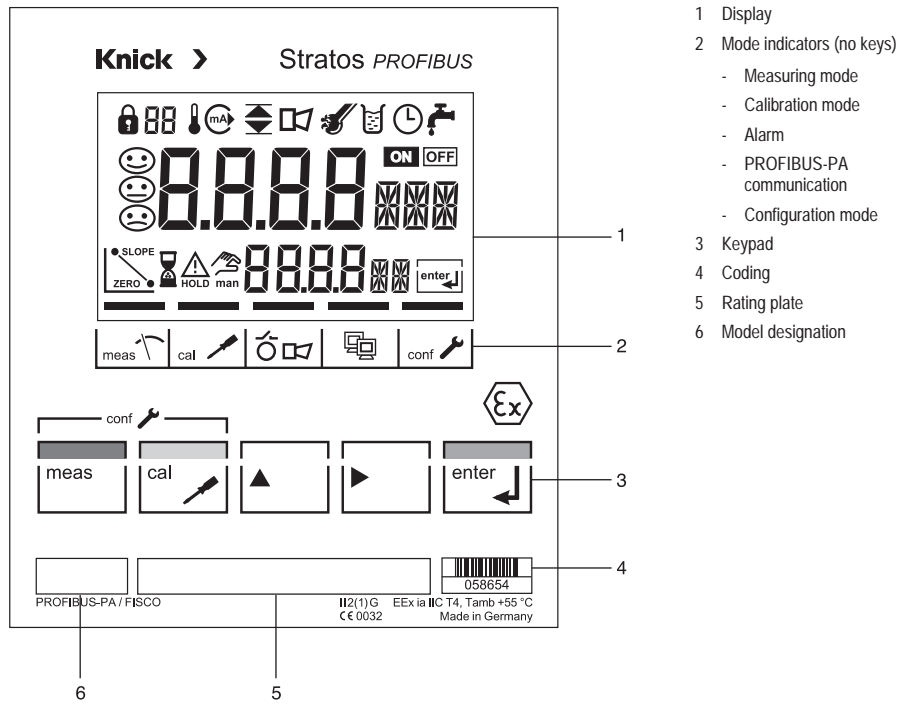


Fig. 8.2 Front view of Stratos


Display

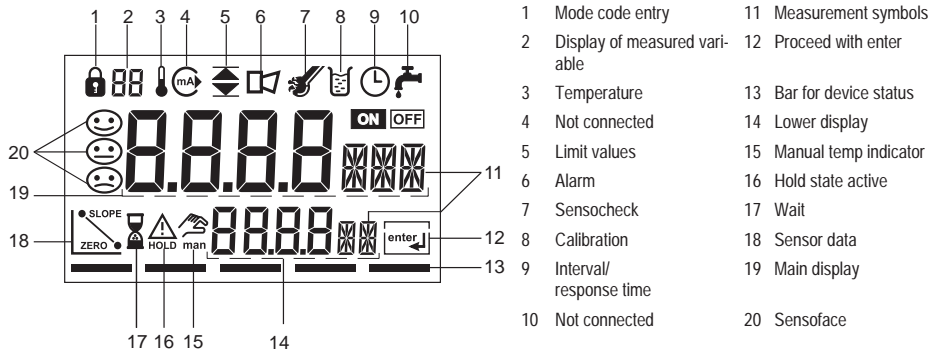

English


Fig. 8.3 Stratos display

Keypad functions

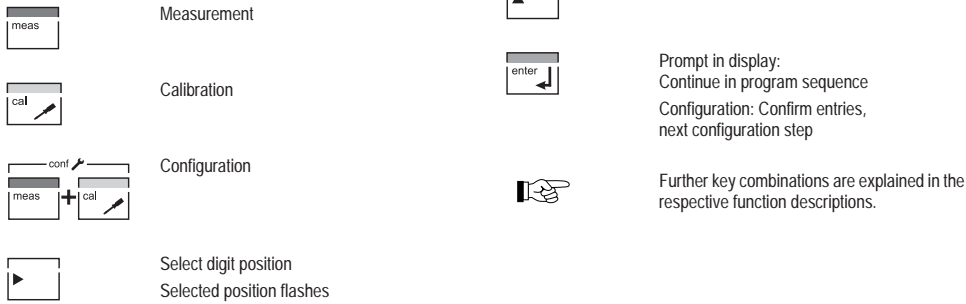

8.3 Mode code

After pressing meas and/or cal you can enter one of the following mode codes to access the designated mode:



conf, 0000	Error Info
conf, 1200	Configuration mode
cal, 1001	Zero point calibration
cal, 1105	Product calibration



cal, 0000	Cal Info
cal, 1015	Adjusting temp probe
cal, 1100	Calibration mode
cal, 2222	Display sensor current (uncompensated)/temperature

8.4 Safety functions

Sensocheck, Sensoface sensor monitoring

Sensocheck monitors the sensor and lines for short circuits or open connections.

Sensocheck can be switched off.

value transfer. It runs automatically in the background at fixed intervals.



Sensoface provides information on the sensor condition.



The zero point, slope and response time during calibration are evaluated.



The three Sensoface indicators provide the user with information about wear and required maintenance of the sensor.

GainCheck manual device self-test

A display test is carried out, the software version is displayed and the memory and measured value transfer are checked.



Start GainCheck manual device self-test

Automatic device self-test

The automatic device self-test checks the memory and measured-

Hold state

The Hold state is a safety state that is activated in the case of interventions such as configuration and calibration. The Stratos freezes the last valid measured value and sends a status message to the control system.



This symbol indicates that the device is in the "Hold" state.

The Hold state is activated by the following mode codes:

- Calibration
 - Mode code 1015 = Temp probe adjustment
 - Mode code 1100 = Calibration mode
 - Mode code 2222 = Display of sensor potential

- Configuration

- Mode code 1200 = Configuration mode

The measured value and Hold are displayed alternately



- Check whether the measured value is plausible
- End the Hold state

After 20 sec (for measured value stabilization) the device returns to measuring mode.

English

8.5 Mode indicators

Measuring mode



The Stratos is in measuring mode.

Calibration mode



Calibration mode is active.

Alarm



During an error message the red alarm LED beneath the display flashes.

The alarm response time is permanently set to 10 sec.

PROFIBUS-PA communication



The Stratos communicates via PROFIBUS-PA and can be configured from the service station. Measured values, messages and device identification can be downloaded at any time. This allows integration in fully automatic process cycles.


Configuration mode



The Stratos is in configuration mode.

8.6 Configuration

In the configuration mode the device parameters are set.
The following steps must be executed:



- Activate configuration



- Enter mode code "1200"



- Confirm



Welcome text 3 sec



During configuration the Stratos remains in the Hold state for reasons of safety.

For configurable parameters, see "Configuration parameters" Page 27.



- Select or edit parameter



- Confirm entries



The configuration parameters are checked during the input.



In the case of an incorrect input "Err" is displayed for 3 sec. The incorrect parameters cannot be stored. Input must be repeated.




- End configuration

The measured value and Hold are displayed alternately.



- End the Hold state / accept configuration or











- Repeat configuration

Configuration parameters

Display	Action	Choices	Factory setting
	Activate configuration (simultaneously press meas and cal)		
	Enter mode code "1200" (Press arrow key ▶ to select position, enter number using ▲ key, confirm with enter)		
	Device is in Hold state. <ul style="list-style-type: none"> Select sensor (type A / B) Proceed with enter Switch over: arrow keys Proceed: enter key 	Sensor Type A (general sensor) Sensor Type B (Mettler InPro6900) Low Level High Level	Type A Hi-Level
	Selection of variable to be displayed <ul style="list-style-type: none"> Switch over: arrow keys Proceed: enter key 	With Low Level selected: µg/l • ppb • mg/l • ppm • % With High Level selected: mg/l • ppm • %	%
	Selection of process temp <ul style="list-style-type: none"> Switch over: arrow keys Proceed: enter key 	man °C / man °F auto °C / auto °F BUS °C / BUS °F: -20 to +150 °C or -4 to +302 °F	Auto °C
	Selection of temp probe (NTC) <ul style="list-style-type: none"> Switch over: arrow keys Proceed: enter key 	Only with Auto selected: 22 kΩ 30 kΩ	22 NTC

English

Display	Action	Choices	Factory setting
	Selection of pressure measurement unit • Switch over: arrow keys • Proceed: enter key	BAR • PSI • KPA	BAR
	Selection of process pressure • Switch over: arrow keys • Proceed: enter key	0.000 to 9.999 bars	1.013 bars
	Selection of salinity • Switch over: arrow keys • Proceed: enter key	00.00 to 45.00 g/kg or %, resp.	00.00
	Selection of polarization voltage • Switch over: arrow keys • Proceed: enter key	0 mV to 800 mV (0 mV = Off)	675 mV
	Selection of Sensocheck On, Off • Switch over: arrow keys • Proceed: enter key	On Off	Off

Display	Action	Choices	Factory setting
	Selection of calibration mode <ul style="list-style-type: none"> Switch over: arrow keys Proceed: enter key 	<ul style="list-style-type: none"> Saturation (Sat) Concentration (Conc) 	Conc
	Selection of cal timer interval		0000 (Off)
	Selection of bus address		126

Tab. 8.1: Configuration parameters

Configuration is circular. To stop, press meas key.

8.7 Calibration

Calibration is used to adapt the device to the DO sensor. Depending on the configuration, the device can be calibrated with regard to saturation or concentration. For each calibration mode, the Stratos suggests useful calibration parameters. Of course, they can be edited as required.

Note:

When a 2-point calibration is required, the zero point calibration should be performed prior to saturation or concentration calibration, resp.



All calibration procedures must be performed by trained personnel.

During calibration, the output current is frozen, limit and alarm contacts are inactive.



Incorrectly set parameters may go unnoticed, but change the measuring properties.

If calibration is exited, the Stratos remains in the Hold state for reasons of safety. The measured value and Hold are displayed alternately. Now you can check whether the measured value is plausible and

specifically end the Hold state with enter or press cal to repeat calibration.

If you end the Hold state, the Stratos will return to measuring mode after 20 sec (for the sensor to adjust).

Zero point calibration







A zero point calibration is not required for most of the biotechnological processes. For these processes, we recommend to set the input current for the zero point to 0.0 nA and then perform a one-point calibration (saturation). If a zero point calibration is performed, the DO

sensor should remain for at least 10 to 30 minutes in the calibration medium in order to obtain accurate values. A drift check is not performed.






Zero point current should be < 0.5 % of air current. The display (secondary: measured value, main: entered value) does not change until an input current is entered for the zero point.

When measuring in an oxygen-free medium, the displayed current can be taken directly.






When the zero point has changed, the slope is automatically adjusted so that the 100% point remains valid.

Display	Zero point calibration – Action	Selection / Remarks
	<ul style="list-style-type: none"> Activate calibration (press cal key) 	
1001	<ul style="list-style-type: none"> Enter mode code "1001" (Press arrow key ▶ to select position, enter number using ▲ key, confirm with enter) Place sensor in oxygen-free medium 	  
	<p>Lower display: actually measured current Main display: value for zero point.</p> <ul style="list-style-type: none"> Confirm with enter or correct using arrow keys and then confirm with enter 	
	<p>Display of slope Display of new zero point</p> <ul style="list-style-type: none"> Place sensor in process End calibration with enter 	<p>After end of calibration, the Stratos remains in Hold state for approx. 20 sec.</p> <p>The oxygen value is displayed.</p>






Saturation calibration

Display	Action	Selection / Remarks
	Select calibration, enter mode code "1100"	cal key, arrow keys
	<ul style="list-style-type: none"> Enter relative humidity Default for aqueous media rH = 100 % Proceed with enter	
	<ul style="list-style-type: none"> Enter calibration pressure, proceed with enter Default: configured process pressure If temperature display follows, temperature can be entered manually, see remarks Proceed with enter 	If "man" or "BUS" has been selected during configuration, the configured process temperature will be displayed. The internal temperature probe is not used.
	<ul style="list-style-type: none"> Automatic drift check: Measurement Display of input current (temperature-compensated) and of measuring temp 	Drift check can be stopped after > 10 sec by pressing cal (accuracy reduced).
	<ul style="list-style-type: none"> Change default value if required 	Default: last value entered
	<ul style="list-style-type: none"> Display of new slope and zero point related to 25°C at 1013 mbars End calibration with enter 	After end of calibration, the oxygen value is displayed for approx. 20 sec. Then the Stratos will return to measuring mode.

Concentration calibration

Display	Action	Selection / Remarks
	Select calibration, enter mode code "1100"	cal key, arrow keys
	Place DO sensor in air for calibration <ul style="list-style-type: none"> Enter relative humidity Proceed with enter 	Default for aqueous media rH = 50 %
	<ul style="list-style-type: none"> Enter calibration pressure, proceed with enter If temperature display follows, temperature can be entered manually, see remarks Proceed with enter 	Default: normal pressure 1013 mbars. If "man" or "BUS" has been selected during configuration, "25 °C" will be displayed. The internal temperature probe is not used.
	<ul style="list-style-type: none"> Measurement Display of input current (temperature-compensated) and of measuring temp 	Drift check can be stopped after > 10 sec by pressing cal (accuracy reduced).
	<ul style="list-style-type: none"> Default value calculated from rel. humidity, cal pressure and cal temp (theoretical concentration for saturation) 	Edit default value if required.
	<ul style="list-style-type: none"> Display of new slope and zero point related to 25 °C at 1013 mbars End calibration with enter 	After end of calibration, the oxygen value is displayed for approx. 20 sec. Then the Stratos will return to measuring mode.

Product calibration

Display	Action	Selection / Remarks
	Select calibration, enter mode code "1105"	cal key, arrow keys
	Product calibration 1st step	Display (approx. 3 sec)
	<ul style="list-style-type: none"> Take sample and store value Proceed with enter 	Now the sample can be measured in the lab. The Stratos is in measuring mode.
	<ul style="list-style-type: none"> Measuring mode While the sample value is determined, the device is in measuring mode. From the flashing CAL mode indicator you see that sample calibration has not been terminated. 	
	<ul style="list-style-type: none"> When the sample value has been determined, call up the product calibration once more (CAL key, mode code 1105). Product calibration 2nd step 	Display (approx. 3 sec)
	Enter lab value. The new slope is calculated. Then zero point and slope are displayed as for ordinary calibration.	Arrow keys

English

Adjusting temp probe



Wrong settings change the measurement properties!

The following steps must be executed:



- Activate calibration
- Enter mode code "1015" and confirm
- Measure the temperature of the process medium using an external thermometer



A welcome text ("CAL TMP") is displayed for 3 sec.

- Then enter the determined temperature value in the main display (arrow keys)

If the value of the main display is set to the value of the secondary display, a correction is not made.

- Confirm with enter



HOLD will be deactivated after 20 sec.

8.8 Operating tool

For parameter setting, commissioning and diagnostics of the Stratos via PROFIBUS, we recommend operating tools such as SIMATIC-PDM Version 5 or higher.

The current device description is included.

8.9 Measurement

Measuring mode

In the measuring mode the main display shows the configured process variable and the lower display the temperature.



The Stratos returns to measuring mode, also from configuration or calibration mode (after a relax time for measured-value stabilization, if required).

Cal Info

"Cal Info" shows the slope and zero point current.



- Activate "Cal Info" function



- Mode code



- Confirm


"Cal Info" shows the current calibration data for approx. 20 sec.



- End "Cal Info"

Error Info

"Error Info" shows the most recent error message.



- Activate "Error Info" function



- Mode code



- Confirm

The error message is displayed for approx. 20 sec. After that the message will be deleted.



- End "Error Info"

9 Diagnostics

9.1 Sensocheck, Sensoface

Three Smileys provide information on wear and required maintenance. This does not affect the measurement process.



Sensoface provides information on the status of the sensor.



The zero point, slope and response time during calibration are evaluated.



A Smiley can only be displayed when Sensocheck has been activated.



The worsening of a Sensoface criterion leads to the devaluation of the Sensoface indicator (average/poor).



An improvement of the Sensoface indicator can only take place after calibration or removal of a sensor defect.








The Sensoface status does not influence the measured value display.



The basis for accurate Sensoface indication is proper calibration.

Sensoface displays

Display	Problem	Status	
	Sensor response time		The sensor adjusts slowly to the measured value. Maybe it has not been polarized sufficiently. You should consider replacing the membrane module and electrolyte.
			The sensor adjusts very slowly to the measured value. Correct measurement is no longer ensured. If this occurs in spite of sufficient polarization, you should replace the membrane module and electrolyte.
	Slope		Sensor slope is still okay. However, membrane module and electrolyte should be replaced soon.
			Sensor slope has reached a value which no longer ensures proper measurement. You should replace membrane module and electrolyte.

Display	Problem	Status	
	Calibration timer		Over 80 % of the calibration interval has already past.
			The calibration interval has been exceeded.
	Sensor defect		Check membrane module and electrolyte and the sensor connections.

English

Tab. 9.1: Sensoface display

9.2 PROFIBUS-PA limit monitoring

Stratos is equipped with two limit blocks that can be separately configured for temperature and/or the process variable.

Configuration is only performed via the bus.

The limit conditions are transmitted cyclically.

Hysteresis, effective direction, on and off delay can be configured.



Limit value setting and output of limit messages is via the PROFIBUS-PA.



When this symbol is displayed, limit block 1 is active.



When this symbol is displayed, limit block 2 is active.

9.3 Error messages

When one of the following error messages is displayed, the device can no longer determine the measured variable correctly.

The alarm response time is permanently set to 10 sec.



During an error message the red alarm LED beneath the display flashes.



The error messages in the display are sorted according to their priority. A higher-priority message overlays a lower-priority message.



Error No.	Display (flashing)	Problem	Possible causes
Err 01		DO sensor	<ul style="list-style-type: none"> - Sensor defect - Incorrect sensor connected - Measurement range (%) exceeded - Current range (mA) exceeded
Err 02		DO sensor	<ul style="list-style-type: none"> - Sensor defect - Measured concentration value lower than 0 mg/l (ppm) or higher than 50 mg/l (ppm)
Err 03		Temperature probe	<ul style="list-style-type: none"> - Open or short circuit in temperature probe - Measured temperature below -10 °C or above +150 °C
Err 33		DO sensor	<ul style="list-style-type: none"> - Membrane defective
Err 98		System error	<ul style="list-style-type: none"> - Configuration or calibration data defective; completely reconfigure and recalibrate the device - Memory error in device program (PROM defective)
Err 99		Factory settings	<ul style="list-style-type: none"> - EEPROM or RAM defective <p>This error message only occurs in the case of a complete defect. The Stratos must be repaired and recalibrated at the factory.</p>

Tab. 9.2: Error messages

Calibration error messages









Calibration error messages only occur during calibration.









Display (flashing)	Problem	Possible causes
	Sensor slope out of range	<ul style="list-style-type: none"> - Wrong calibration values specified (relative humidity, pressure, saturation, concentration)
	Calibration was canceled after approx. 12 minutes, because the sensor drift was too large.	<ul style="list-style-type: none"> - Sensor defective or dirty - No electrolyte in the sensor - Sensor cable insufficiently shielded or defective - Strong electric fields influence the measurement - Temperature fluctuation of calibration solution

English

Tab. 9.3: Calibration error messages

9.4 Display messages and PROFIBUS communication

User interface / display of device				Cause For comments see Pg 38 through Pg 39	Communication via PROFIBUS				
Display pictograph	Display message	Sensoface	LED		No. of binary message (logbook)	Analog input status	Physical Block (PB) Global status	Text of binary message (factory setting)	Logbook entry (factory setting)
	Err 99		X	Factory settings defective	1	0000 11xx	Failure	ERR SYSTEM	X
	Err 98		X	Configuration data defective, Gaincheck	2	0000 11xx	Failure	ERR PARAMETERS	X
	Err 98		X	Memory error (RAM, ROM, EPROM)	3	0000 11xx	Failure	ERR MEMORY	X
	Err 01		X	Measurement range violation	4	0100 0111 0100 1111	Failure	ERR SAT VALUE	X
	Err 02		X	Measurement range violation	5	0100 0111 0100 1111	Failure	ERR CONC VALUE	X
	Err 03		X	Temp range violation Temperature probe	6	0100 0111 0100 1111	Failure	ERR TEMP VALUE	X
	Err 33		X	Membrane defective	7	0100 0111 0100 1111	Failure	ERR SENSOCHECK	X

User interface / display of device				Cause	Communication via PROFIBUS				
Display pictograph	Display message	Sensoface	LED	For comments see Pg 38 through Pg 39	No. of binary message (logbook)	Analog input status	Physical Block (PB) Global status	Text of binary message (factory setting)	Logbook entry (factory setting)
				Zero point/ Slope	8	0101 00xx	Maintenance required	CHK ZERO/SLOPE	X
				Sensor response time	9	0101 00xx	Maintenance required	CHK EL. RESPONSE	X
				Calibration timer Cal prompt	10	0101 00xx	Maintenance required	CAL REQUIRED	X
				Calibration	11	0100 0111 0100 1111	Function check	CAL RUNNING	X
				Configuration	12	0100 0111 0100 1111	Function check	CONF RUNNING	X
				HOLD (Device state = Maintenance)	13	0100 0111 0100 1111	Function check	HOLD	X
				HI_HI_LIM FB analysis	14	1000 1110	Limit 1 Bit 1	HI_HI_LIMIT OXY	
				HI_LIM FB analysis	15	1000 1010	Limit 1 Bit 2	HI_LIMIT OXY	
				LO_LIM FB analysis	16	1000 1001	Limit 1 Bit 3	LO_LIMIT OXY	

English

User interface / display of device				Cause	Communication via PROFIBUS				
Display pictograph	Display message	Sensoface	LED	For comments see Pg 38 through Pg 39	No. of binary message (logbook)	Analog input status	Physical Block (PB) Global status	Text of binary message (factory setting)	Logbook entry (factory setting)
				LO_LO_LIM FB analysis	17	1000 1101	Limit 1 Bit 4	LO_LO_LIMIT OXY	
				HI_HI_LIM FB temperature	18	1000 1110	Limit 2 Bit 1	HI_HI_LIMIT TEMP	
				HI_LIM FB temperature	19	1000 1010	Limit 2 Bit 2	HI_LIMIT TEMP	
				LO_LIM FB temperature	20	1000 1001	Limit 2 Bit 3	LO_LIMIT TEMP	
				LO_LO_LIM FB temperature	21	1000 1101	Limit 2 Bit 4	LO_LO_LIMIT TEMP	
				Logbook empty	22		Function check	EMPTY LOGBOOK	

Tab. 9.4: Display messages and PROFIBUS communication

9.5 Diagnostics functions

Cal Info

"Cal Info" shows the slope and zero point current.



- Activate "Cal Info" function



- Mode code



- Confirm


The current calibration data are displayed for approx. 20 sec.



- End "Cal Info"

Error Info

"Error Info" shows the most recent error message.



- Activate "Error Info" function



- Mode code



- Confirm

The error message is displayed for approx. 20 sec. After that the message will be deleted.



- End "Error Info"

Display of sensor current




This symbol indicates that the temperature will be manually specified.

During sensor maintenance it is useful to directly indicate the sensor current. This allows, for example, to check sensor response after cleaning.



- Select function



- Enter mode code "2222"



- Confirm

The sensor current is displayed.



- End display mode



During sensor current display the Stratos is in the Hold state.

GainCheck manual device self-test

A display test is carried out, the software version is displayed and the memory and measured value transfer are checked.

 • Start GainCheck manual device self-test

Automatic device self-test

The automatic device self-test checks the memory and measured-value transfer. It runs automatically in the background at fixed intervals.

10 Maintenance and cleaning

10.1 Maintenance

The Stratos contains no user repairable components.

10.2 Cleaning

To remove dust, dirt and spots, the external surfaces of the Stratos may be wiped with a soft cloth moistened with water.

A mild household cleaner may also be used if necessary.

English

11 Appendix

11.1 Product line

Devices

Model designation	Ref. No.
Stratos PROFIBUS 2221 X Oxy for hazardous- and safe-area applications	2221 X Oxy

Mounting accessories

Accessories	Ref. No.
Pipe-mount kit	ZU 0274
Panel-mount kit	ZU 0275
Protective hood	ZU 0276

11.2 Specifications

General specifications

Manufacturer / ID	Knick Elektronische Meßgeräte GmbH / KNIC
Model designation / ID	Stratos PROFIBUS 2221 X Oxy / 2533

Applications

Measurement of dissolved oxygen and temperature

DO input	Input for SE704/SE705, Inpro6000 dissolved oxygen sensors	
Range 1 (low level)	Measuring current	-2 to +600 nA, resolution 10 pA
	Saturation (-10 °C to +80 °C)	0.0 to 120.0 %
	Meas. error ^{1,2,3}	0.5 % meas. value + 0.1 % saturation
	Concentration (-10 °C to +80 °C)	0000 to 9999 µg/l 0000 to 9999 ppb 0000 to 9999 ppm 0000 to 9999 mg/l
	Meas. error ^{1,2,3}	0.5 % meas. value + 5 µg/l or 5 ppb, resp.
Range 2 (high level)	Measuring current	-2 to +1800 nA, resolution 30 pA
	Saturation (-10 °C to +80 °C)	0 to 500 %
	Meas. error ^{1,2,3}	0.5 % meas. value + 0.5 % saturation
	Concentration (-10 °C to +80 °C)	0.0 to 50.00 mg/l 0.0 to 50.00 ppm
	Meas. error ^{1,2,3}	0.5 % meas. value + 50 µg/l or 50 ppb, resp.
Polarization voltage	0 to 1000 mV	
Process pressure	0.000 to 9.999 bars 999.9 kPa 145.0 psi	
Salt correction	0.00 to 45.00 g/kg	
Sensocheck	Monitoring for short circuits or open circuits (can be disabled)	

Sensor standardization (cal)	Zero point calibration Calibration with entry of oxygen saturation Calibration with entry of oxygen concentration at saturation Product calibration	
Calibration range	Zero	± 2 nA
	Slope	Sensor Type A: 25 to 130 nA Sensor Type B: 200 to 550 nA (Mettler-Toledo InPro6900)
Cal timer*	0 to 9999 h	
Pressure correction	Calibration pressure to be entered manually or via PROFIBUS	
Temperature input	NTC 22kΩ or NTC 30 kΩ, 2-wire connection, ± 5 K adjustable	
Range	-20.0 to +150.0 °C / -4 to +302 °F	
Resolution	0.1 °C / 1 °F	
Meas. error ^{1,2,3}	< 0.5 K (< 1 K bei > 100 °C)	
Temperature compensation	Automatic with NTC or manual temperature	
Logbook	Recording of error messages	
Storage capacity	40 entries, can be read out via Profibus (see profile description)	
Limit values	Cyclical discrete signal (DI) via Profibus (see profile description) User-defined via Profibus for: Oxygen saturation Oxygen concentration Temperature	
Alarms and messages	Binary messages to PNO profile 3.0 Signalling via PROFIBUS and logbook entry	

*) Configurable

1) To IEC 746 Part 1, at nominal operating conditions

2) ± 1 count

3) Plus sensor error

Conditions for use

Temperature	Operation	-20 to +55 °C	
	Transport and storage	-20 to +70 °C	
Electromagnetic compatibility	Emitted interference	EN 61 326 Class B	
	Immunity to interference	EN 61 326, EN 61 326/A1	
Ingress protection	Enclosure	IP 65	
Explosion protection	PROFIBUS-PA according to FISCO model of PTB	II 2(1) G EEx ia IIC T4, FISCO	
	FM	IS, Class I Div1, Group A, B, C, D T4 FISCO I / 1[0] / AEx ib [ia] / IIC / T4 FISCO NI, Class I Div2, Group A, B, C, D T4 NIFW	
Data retention	Parameters and calibration data	> 10 years	EEPROM

English

Construction

Dimensions	Height	144 mm	
	Width	144 mm	
	Depth	105 mm	
Weight	Approx. 1 kg		
Material	PBT (polybutylene terephthalate)		
Color	Bluish gray	RAL 7031	
Assembly	Wall mounting		
	Post/pipe mounting	on pipe with 40 to 60 mm diameter, on square post with 30 to 45 mm edge length	
	Panel mounting	Cutout to DIN 43 700 Sealed against panel	
Electrical connection	Cable glands	3 breakthroughs	for included cable glands
		2 breakthroughs	for NPT 1/2" or Rigid Metallic Conduit or cable glands






Display and user interface

Display	LC display, 7-segment	Measured value display	µg/l, mg/l, ppb, ppm, %, temperature
		3 Sensoface states	Good / average / poor
		5 mode indicators	meas / cal / alarm / online / conf
	Alarm LED	Error message	
Operation	5 keys	meas / cal / up / right / enter	
Operating tool	Device description (DD) implemented in SIMATIC PDM		

Interface

PROFIBUS-PA communication	Digital communication by current modulation of supply current Reading of device identification, measured values, status and message Reading and writing of parameter and configuration data	
	Protocol	PROFIBUS-PA (DPV1)
	Connection	Via segment coupler to SPC, PC, PCS
	Profile	PNO directive: PROFIBUS-PA, Profile for Process Control Devices, Version 3.0
	Physical interface	To IEC 1158-2
	Address range	1 to 126, default: 126
	Supply voltage	FISCO bus supply: 9 to 17.5 V Linear barrier: 9 to 24 V
	Current consumption	< 13.2 mA
	Max. current in case of fault (FDE)	< 17.6 mA

English

	Prüf- und Zertifizierungsstelle ZELM Ex	
(1) EC-TYPE-EXAMINATION CERTIFICATE (Translation)		
(2) Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres - Directive 94/9/EC		
(3) EC-TYPE-EXAMINATION CERTIFICATE Number: ZELM 01 ATEX 0069		
(4) Equipment:	Transmitter Stratos PROFIBUS 2221 X Oxy	
(5) Manufacturer:	Knick Elektronische Meßgeräte GmbH & Co.	
(6) Address:	D - 14163 Berlin, Beuckestraße 22	
(7) This equipment and any acceptable variation thereto are specified in the schedule to this certificate and the documents therein referred to.		
(8) The Prüf- und Zertifizierungsstelle ZELM Ex, notified body No. 0820 in accordance with Article 9 of the Council Directive 94/9/EC of 23 March 1994, certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment and protective systems intended for use in potentially explosive atmospheres, given in Annex II to the Directive. The examination and test results are recorded in the confidential report ZELM Ex 0290112097.		
(9) Compliance with the Essential Health and Safety Requirements has been assured by compliance with: EN 50 014: 1997+A1+A2 EN 50 020: 1994		
(10) If the sign "X" is placed after the certificate number, it indicates that the equipment is subject to special conditions for safe use specified in the schedule to this certificate.		
(11) This EC-type-examination Certificate relates only to the design and construction of the specified equipment in accordance with Directive 94/9/EC. Further requirements of this Directive apply to the manufacture and supply of this equipment.		
(12) The marking of the equipment shall include the following:		
 II 2 (1) G EEx ia IIC T4		
Zertifizierungsstelle ZELM Ex		Braunschweig, November 21, 2001
 Dipl.-Ing. Harald Zelm		Sheet 1/3
EC-type-examination Certificates without signature and stamp are not valid. The certificates may only be circulated without alteration. Extracts or alterations are subject to approval by the Prüf- und Zertifizierungsstelle ZELM Ex. In case of dispute, the German text shall prevail. Prüf- und Zertifizierungsstelle ZELM Ex • Siekgraben 56 • D-38124 Braunschweig		



SCHEDULE

(13)

(14) EC-TYPE-EXAMINATION CERTIFICATE ZELM 01 ATEX 0069

(15) Description of equipment

The Transmitter Stratos PROFIBUS 2221 X Oxy with Profibus - PA - communication interface is preferably used for the recognition and processing of electrochemical quantities and is equipped with an input for measurements of the oxygen partial pressure and a temperature measuring input.

The maximum permissible ambient temperature is 55 °C.

Electrical data

BUS- / Supply loop (terminals 11 and 10)

type of protection Intrinsic Safety resp. EEx ia IIC/IIB EEx ib IIC/IIB

for the connection to a certified intrinsically safe circuit only (for example FISCO - supply unit) with the following maximum values:

	FISCO- supply unit	linear barrier
U_{max}	17.5 V	24 V
I_{max}	280 mA	200 mA
P_{max}	4.9 W	1.2 W

effective internal capacitance: $C_i \leq 1$ nF

effective internal inductance: $L_i \leq 10$ µH

Oxygen measuring loop (terminals 1/2, 4 and 5)

type of protection Intrinsic Safety resp. EEx ia IIC/IIB EEx ib IIC/IIB

maximum values:

$U_o = 10$ V

$I_o = 11$ mA

$P_o = 14$ mW

$R = 475$ Ω

(linear characteristics)


	IIC	resp.	IIB
max. permissible external inductance	1 mH		5 mH
max. permissible external capacitance	925 nF		4 µF

effective internal capacitance: $C_i \leq 25$ nF
The effective internal inductance is negligibly small.


Sheet 2/3

EC-type-examination Certificates without signature and stamp are not valid. The certificates may only be circulated without alteration. Extracts or alterations are subject to approval by the Prüf- und Zertifizierungsstelle ZELM Ex. In case of dispute, the German text shall prevail.

Prüf- und Zertifizierungsstelle ZELM Ex • Siekgraben 56 • D-38124 Braunschweig



Prüf- und Zertifizierungsstelle
ZELM Ex



SCHEDULE TO EC-TYPE-EXAMINATION CERTIFICATE ZELM 01 ATEX 0069

Temperature measuring loop (terminals 7 and 8)	type of protection Intrinsic Safety resp. maximum values:	EEx ia IIC/IIB EEx ib IIC/IIB $U_s = 5 \text{ V}$ $I_i = 1 \text{ mA}$ $P_s = 2 \text{ mW}$ $R = 7,88 \text{ k}\Omega$ (linear characteristics)												
		<table border="0" style="margin: auto;"> <tr> <td></td> <td style="text-align: center;">IIC</td> <td style="text-align: center;">resp.</td> <td style="text-align: center;">IIB</td> </tr> <tr> <td>max. permissible external inductance</td> <td style="text-align: center;">1</td> <td style="text-align: center;">mH</td> <td style="text-align: center;">5</td> </tr> <tr> <td>max. permissible external capacitance</td> <td style="text-align: center;">4</td> <td style="text-align: center;">µF</td> <td style="text-align: center;">10</td> </tr> </table>		IIC	resp.	IIB	max. permissible external inductance	1	mH	5	max. permissible external capacitance	4	µF	10
	IIC	resp.	IIB											
max. permissible external inductance	1	mH	5											
max. permissible external capacitance	4	µF	10											
		effective internal capacitance: $C_i \leq 120 \text{ nF}$ The effective internal inductance is negligibly small.												


EP
(terminal 9) for the connection to the equipotential bonding system


References:
 Connecting the equipotential bonding is absolutely required to guarantee electrostatic leakage.
 The BUS- / Supply loop is safely electrically isolated from the other loops up to a peak value of the nominal voltage of 60 Volts.
 The operation manual has to be considered.

(16) **Report No.** ZELM Ex 0290112097

(17) **Special conditions for safe use**
not applicable

(18) **Essential Health and Safety Requirements**
met by standards


 Dipl.-Ing. Harald Zelm




Braunschweig, November 21, 2001

Sheet 3/3

EC-type-examination Certificates without signature and stamp are not valid. The certificates may only be circulated without alteration. Extracts or alterations are subject to approval by the Prüf- und Zertifizierungsstelle ZELM Ex. In case of dispute, the German text shall prevail.

Prüf- und Zertifizierungsstelle ZELM Ex • Siekgraben 56 • D-38124 Braunschweig


11.4 Provided documentation:



- Instruction manual



- Safety instructions /
EC Declarations of Conformity



- Short instructions

Devices only:



- EC-Type Examination Certificate

Oxy Transmitter
 Stratos PROFIBUS PA 2221 X Oxy
 Stratos FF 2231 X Oxy
 IS/II/ABCO/T4, Ta=55°C, Entity, FISCO
 I/II/AEx ib I/II/IC/T4, Ta=55°C, Entity, FISCO

Entity Parameters:

Terminals 1/2, 4, 5 and 6
 $V_L = 10\text{ V}$ $C_d = 925\text{ nF}$
 $I_L = 11\text{ mA}$ $L_d = 1\text{ mH}$
 $P_{max} = 14\text{ mW}$

Terminals 7 and 8
 $V_{oc} = 5\text{ V}$ $C_d = 4\text{ nF}$
 $I_{sc} = 1\text{ mA}$ $L_d = 1\text{ H}$
 $P_{max} = 2\text{ mW}$

The intrinsically safe equipment connecting to 1, 2, 4, 5, 6 and 7, 8 must be FM Approved or be simple apparatus, a device which will neither generate nor store more than 15 V, 0.1 A, 25 mW.

O₂ sensor series InPro 6xxx

Cable max 10 m

Table 1

Concept	Groups	V _{max} [V]	I _{max} [mA]	P _{max} [W]	C _d [nF]	L _d [mH]	µPFD
Entity	IC/ABCD	24	200	12	12	7	
FISCO	IC/ABCD	17.5	280	4.9			

FISCO rules
 The FISCO Concept allows the interconnection of intrinsically safe apparatus to associated apparatus not specifically approved for such combinations. The criteria for such combinations are: Maximum voltage (V_{max}), the current (I_{max}) and the power (P) which intrinsically safe apparatus can receive and which intrinsically safe cables can carry, must be equal or greater than the voltage (V_L, I_L, P_L), the current (I_{sc}, I_{sc}) and the power (P_{oc}) which can be provided by the associated apparatus (simple or not). In addition, the maximum operational inductance (L_d) and capacitance (C_d) of each apparatus (other than the terminator) connected to the FISCO must be less than or equal to 5 nF and 10 µH respectively.

In each IS, FISCO segment only one active source, normally the associated apparatus, is allowed to provide the necessary power for the FISCO system. The allowed voltage (V_L, I_L, P_L) of the associated apparatus must be equal to or greater than the voltage (V_{max}, I_{max}, P_{max}) of the other equipment connected to the bus cable has to be possible, meaning that the apparatus is not allowed to provide energy to the system, except for leakage current of 1 µA for each connected device. Separately powered equipment needs a galvanic isolation to ensure that the intrinsically safe FISCO circuit remains passive.

The cable used to interconnect the devices needs to comply with the following parameters:
 Loop inductance L_d ≤ 100 nH/m
 Inductance per unit length L_d ≤ 0.4 - 1 nH/m
 Capacitance per unit length C_d ≤ 200 nF/m
 C_d ≤ 4 nF/meter + 0.5 nF/connector (if both lines are floating)
 C_d ≤ 4 nF/meter + 0.5 nF/connector, if the screen is connected to one line
 Length of loop cable max. 30 m
 Length of bus cable max. 1 km
 Length of splice max. 1 m

Terminations
 Attach end of the bus cable an approved line terminator with the following parameters is suitable:
 R = 90 - 100 Ω
 C_d ≤ 1 - 2 µF

System installation
 The number of passive devices (the transmitters, indicators, connected to a single bus segment) is not limited to 10. However, furthermore, if the above rules are respected, the inductance and capacitance of the cable used need to be considered and will not impair the intrinsic safety of the installation.

Installation Notes For FISCO and Entity Concepts

- The Intrinsic Safety Entity concept allows the interconnection of FM Approved intrinsically safe devices with entity parameters not specifically mentioned in combination as a system when:
 - Use of V_L or I_L or P_L is not allowed. C_d or L_d or µPFD are not allowed.
 - The intrinsic safety FISCO concept covers the interconnection of the approved intrinsically safe devices with FISCO parameters not specifically mentioned in combination as a system when:
 - Use of V_{max}, I_{max}, or P_{max} is not allowed.
 - Use of C_d or L_d or µPFD is not allowed.
- Double-light conduct cables must be used when installed in Class II and Class III environments.
- Control equipment connected to the Associated Apparatus must not use or generate more than 250 V rms or V_{oc}.
- Installations should be in accordance with ANSI/ISA 818.01 (except chapter 4 for FISCO installations), "Installation of Intrinsically Safe Systems for Hazardous (Classified) Locations" and the National Electrical Code (ANSI/NFPA 70) Sections 504 and 505.
- The configuration of associated apparatus must be FM Approved under the associated concept.
- Associated Apparatus manufacturer's installation drawings must be followed when installing this equipment.
- The Stratos FF Series are Approved for Class I, Zone 1, Div. 1 applications, if connecting AEx II(1) associated Apparatus or AEx II, I.E. Apparatus to the Stratos PA, Stratos FF Series (I.E. which is only suitable for Class I, Zone 1, Div. 1, Class 2, and is not suitable for Class I, Zone 0 or Class 1, Division 1, Hazardous (Classified) Locations).
- No revision to drawing without prior FM Approval authorization.
- Simple Apparatus is defined as a device that does not generate more than 15 V, 0.1 A or 25 mW.

Diagram showing terminal connections 1-8 and a note: "Parameters see table 1".

Labels: "Any FM Approved Associated Apparatus", "Any FM Approved Terminator (May not be necessary for Entity Installations)", "Unclassified Locations", "Hazardous (Classified) Locations Class I, Zone 1, Group IC Class I, Division 1, Groups A, B, C and D", "Stratos PROFIBUS PA 2221 X Oxy Stratos FF 2231 X Oxy", "Any FM Approved Intrinsically Safe Apparatus", "Any FM Approved Terminator (May not be necessary for Entity Installations)".

Diagram showing terminal connections 1-8 and a note: "Parameters see table 1".

Labels: "Any FM Approved Associated Apparatus", "Any FM Approved Terminator (May not be necessary for Entity Installations)", "Unclassified Locations", "Hazardous (Classified) Locations Class I, Zone 1, Group IC Class I, Division 1, Groups A, B, C and D", "Stratos PROFIBUS PA 2221 X Oxy Stratos FF 2231 X Oxy", "Any FM Approved Intrinsically Safe Apparatus", "Any FM Approved Terminator (May not be necessary for Entity Installations)".

Version: 01 (01)	Ziel: Anzeigegerät für Methan-Intercompteur	Herstellung: 03.05.04	Modell: 194,470-120	Seite: 1/2
	Zeichner: [Name]	Gezeichnet: 03.10.04	Geprüft: [Name]	
	Gezeichnet: 03.10.04	Geprüft: [Name]		
	Gezeichnet: 03.10.04	Geprüft: [Name]		
	Gezeichnet: 03.10.04	Geprüft: [Name]		
	Gezeichnet: 03.10.04	Geprüft: [Name]		
	Gezeichnet: 03.10.04	Geprüft: [Name]		
	Gezeichnet: 03.10.04	Geprüft: [Name]		

Knick >
 Industrietechnik GmbH & Co. KG (0305) 470-120
 E-Mail: info@knick.de

English

12 Index

A

Analog Input (AI) Function Block, E-10
Applications, E-46

Assembly

Enclosure, E-11
Panel-mount kit (ZU 0275), E-13
Pipe-mount kit (ZU 0274), E-13
Protective hood (ZU 0276), E-14
Stratos, E-12

C

Cal Info, E-35, E-43
Calibration, E-29
 Sensoface, E-36
Calibration error message, E-39
Certificate of Conformity, E-51

Cleaning

Stratos, E-45

Commissioning, E-20

Conditions for use, E-48

Configuration, E-26

Connection, E-15

 Examples, E-18

 Lines, E-16

Construction, E-49

Control Transducer Block, E-9

D

Declaration of Conformity, E-54

Device description, E-7

Device self-test

 Automatic, E-24, E-44

 Manual, E-24, E-44

Diagnostics functions, E-43

Discrete Input (DI) Function Block, E-10

Display, E-23

Display messages and PROFIBUS communication, E-40

Display sensor current, E-43

Dissolved oxygen measurement, E-18

Division 2 wiring, E-15

E

Error Info, E-35, E-43

Error message, E-38

 Calibration, E-39

Explosion protection, E-4

F

FM Control Drawing, E-55

G

GainCheck, E-24, E-44

H

Hold state, E-25

English

I	Process variable
Information	Configuring, E-27
Installation, E-15	Product line
Instruction manual, E-3	Devices, E-46
Installation, E-15	Mounting accessories, E-46
K	PROFIBUS
Keypad functions, E-23	Variations, E-5
L	PROFIBUS technology, E-5
Limit monitoring	PROFIBUS-PA
PROFIBUS-PA, E-37	Definitions, E-6
Logbook, E-10	Limit monitoring, E-37
Logbook Function Block, E-10	Proper use, E-7
M	Protective hood (ZU 0276), E-14
Maintenance	S
Stratos, E-45	Safety functions, E-24
Measurement, E-35	Safety information, E-4
Mode code, E-24, E-61	Sensocheck, E-24, E-36
Mode indicators, E-25	Sensoface, E-24, E-36
Mounting plan, E-12	Calibration, E-36
O	Sensor monitoring, E-24
Operation possibilities, E-21	Specifications, E-46
P	Stratos
Package contents, E-11	Overview, E-17
Panel-mount kit (ZU 0275), E-13	Stripping lengths, E-16
Physical Block (PB), E-9	T
Pipe-mount kit (ZU 0274), E-13	Technical features, E-7
	Temperature specification
	Manual, E-43


Terminal assignments, E-17
Transducer Alarm Block, E-10
Transducer Block (TB), E-9
Transducer Limit Block, E-9
Transfer Transducer Block, E-9
Type Examination Certificate, E-51, E-53

U

Unpacking, E-11
User interface, E-22

English

Mode code



conf, 0000 Error Info
 conf, 1200 Configuration mode



cal, 0000 Cal Info
 cal, 1001 Zero point calibration
 cal, 1015 Adjusting temp probe
 cal, 1100 Calibration mode
 cal, 1105 Product calibration
 cal, 2222 Display sensor current (uncompensated)/
 temperature

Knick
Elektronische Meßgeräte
GmbH & Co.
P. O. Box 37 04 15
D-14134 Berlin
Germany

Tel: +49 (0)30 - 801 91 - 0
Fax: +49 (0)30 - 801 91 - 200
www.knick.de
knick@knick.de

TA-194.470-KNX02